



Quick start guide Jelly Bean Switch

Mini Monitor with Lead




Any questions? Call us on +353 (0)1 247 9007

Jelly Bean Switch Activation

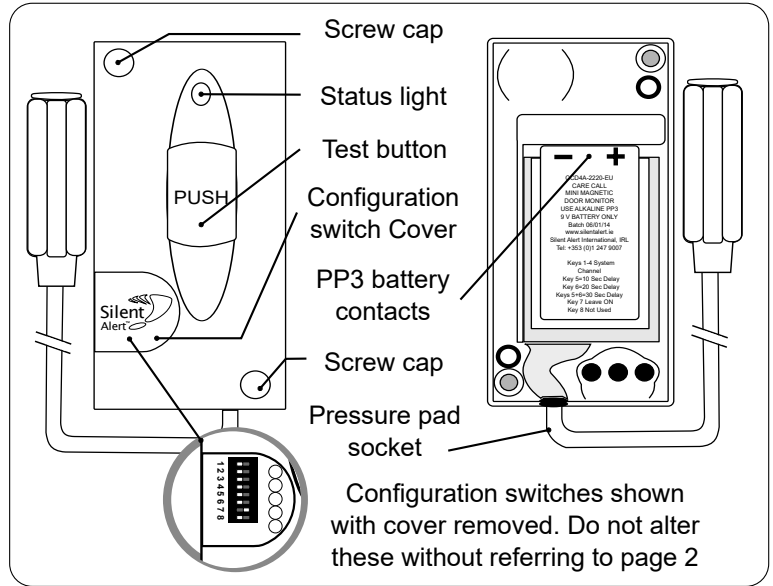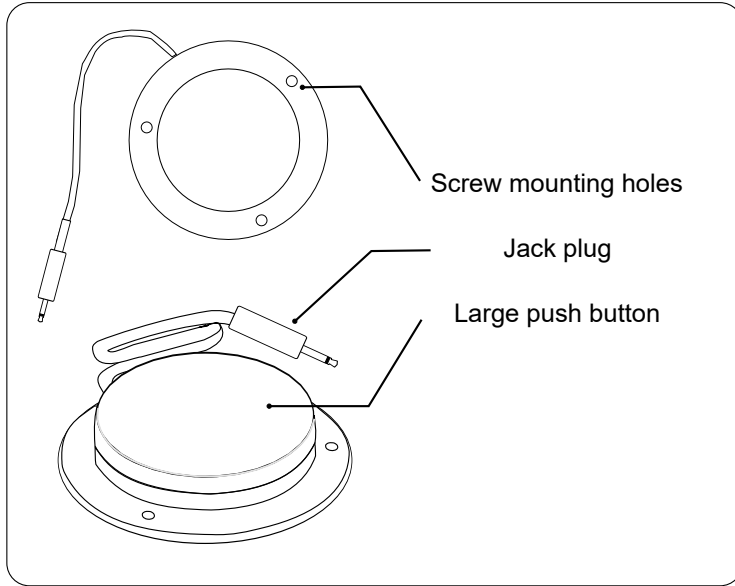

2. Install a 9 volt PP3 alkaline or lithium battery making sure to observe the correct polarity.

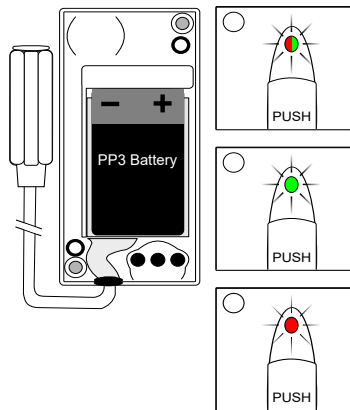

When a battery is first fitted the indicator light will flash red then green a few times then light solid green & pause briefly.


The light will then will flash green several times to show the battery voltage.
9 flashes = 9Volts in the battery.

If the light flashes red at this point the battery is flat and will need to be replaced.


To repeat the battery check remove the battery, press the test button then re-insert the battery to start the sequence again.

3. The monitor is activated using a jelly bean switch.

Plug the switch plug into the socket on the monitor.




The connection can be taped for added security if required.



The monitor may transmit the first time the connection is made, this is normal.


4. Place the switch on a bedside table or similar flat, stable surface.



WARNING

When installing the switch make sure the cable doesn't cause a trip hazard.

5. Alternatively the switch could be mounted to a wall using the mounting holes in the base.



Advanced settings Jelly Bean Switch

Mini Monitor with Lead


Any questions? Call us on +353 (0)1 247 9007

It is possible for the monitor to light up different keys on the Pager or SignWave. This allows more than one mini monitor to be used on a SA3000 system.

Move the relevant key to the right.

Press the test button and check the correct event is received by the Pager or SignWave.

Key 7 must be left on.

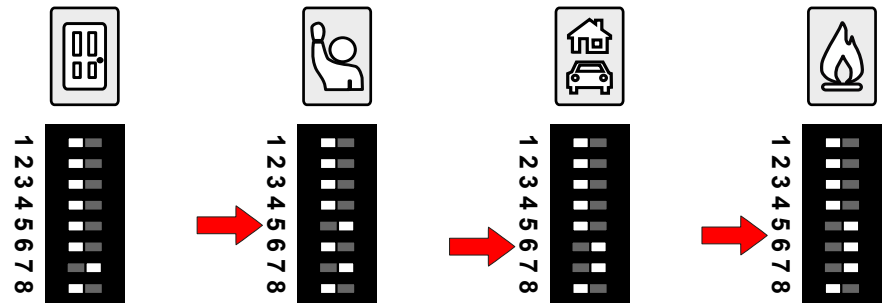

Changing the system channel code


NOTE. In most cases it is not necessary to change the system code. However, when one or more systems are in close proximity, system codes can be used to avoid interference from other SA3000 systems using up to a maximum of 16 channels.

The monitor is supplied with no system code switches set (system code 1). For reference this is the factory setting should you need to re-set the unit.

System codes can be set using key switches 1 - 4.

The diagram to the right shows the 16 possible combinations.

Be sure that the same system code is set on the receiver to be used and any other monitoring options in that system.

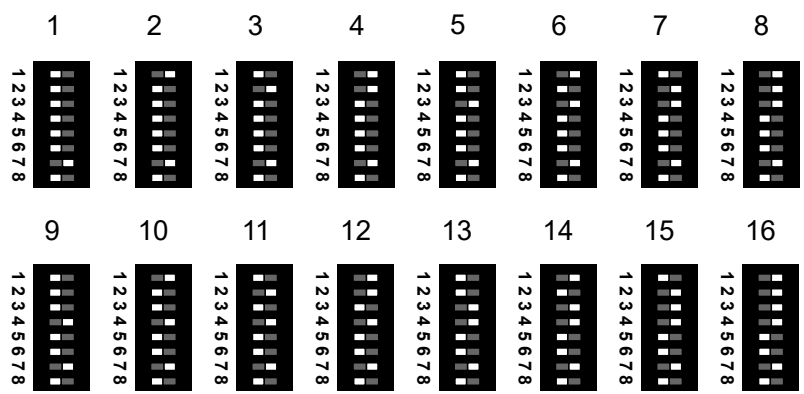

KEY 7 MUST BE LEFT ON!